

2810 Clark Avenue • St. Louis, MO 63103-2574 • (314) 531-8080 • FAX (314) 531-8085
Chemical, Metallurgical, Mechanical, Nondestructive, Environmental Testing, Analyses and Field Service.

RC IMAGING
 50 Old Hojack Lane
 Hilton, NY 14468


January 11, 2016
 Lab No. 16P-0122
 Invoice No. 209305
 Page 1 of 1
 (Revised Report 1/14/16)

Attention: Brian Meyer

REPORT OF MECHANICAL TESTS

SAMPLE ID: 1 Each, #1 Carbon Fiber Cover WBC1417-700 Rev C
SUBJECT Weight Bearing Case (WBC) Load Test
SPECIFICATION: Tested per Clause 9.8.3.2 a) of IEC 60601-1:2005 +A1:2012 per client's directions
PROCEDURE: A 14" diameter disk was placed on Sample, and Loaded to 1500lbs for 1 minute.
TEST INSTRUMENT: Instron Model 5500R w/ Bluehill 3 Software(Cal Due 3/16)
RESULTS: Specimen was not damaged during testing.

Rated Load (lbs)	Load Applied (lbs)
750	1500

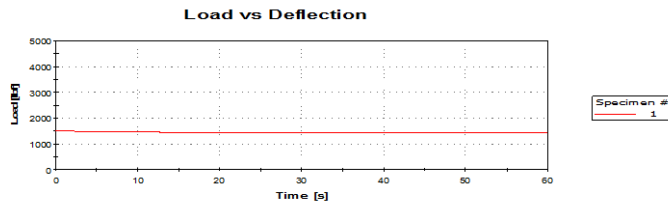

KS/jlm

Karl Schmitz, Director
 Materials Testing



Certificate No. 0397-01
 Certificate No. 0397-02

